


Step by step instructions


HB 142 / HB 342 / ERY 142 / HCT 142




1. Insert capillary with blood sample into cuvette

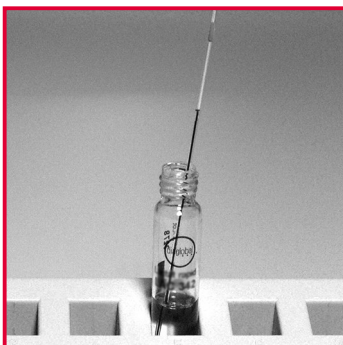


2. Wash out blood with micropipetter

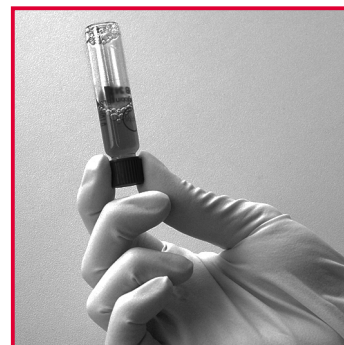


3. Screw on cap
Turn cuvette upside down several times
Wait 3 minutes
HB 342: wait 30 seconds

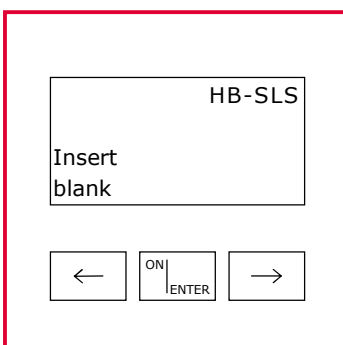


4. Switch on photometer with ON/ENTER
Wait for device check, confirm with ON/ENTER
Select the required test, confirm with ON/ENTER

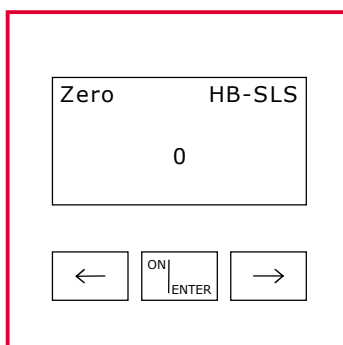

5. Blank adjustment:
Insert non-treated cuvette from package into photometer
Blank is stored in memory

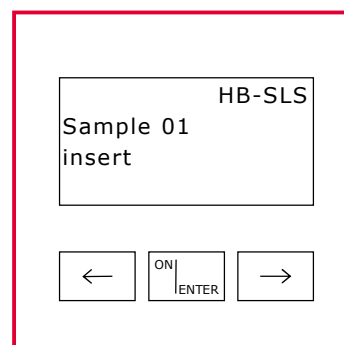

6. Remove cuvette after signal tone

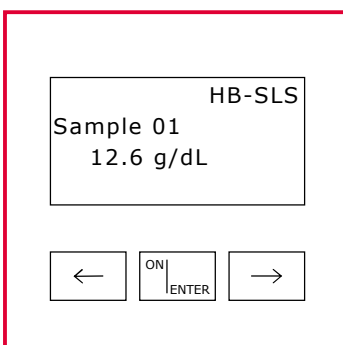

7. Insert cuvette with blood sample (fig. 3) into photometer
Read result



In regard to serial measurement

After blank setting any number of additional samples can be measured